

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
2 June 2005 (02.06.2005)

PCT

(10) International Publication Number
WO 2005/049124 A1

(51) International Patent Classification⁷: A61M 16/22,
16/00, 16/01

(72) Inventor; and
(75) Inventor/Applicant (for US only): PSAROS, Georgios
[SE/SE]; Sågstuguvägen 31, S-146 38 Tullinge (SE).

(21) International Application Number:
PCT/SE2004/001613

(74) Agent: ALBIHNS STOCKHOLM AB; Linnégatan 2,
P.O. Box 5581, S-114 85 Stockholm (SE).

(22) International Filing Date:
8 November 2004 (08.11.2004)

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN,
CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI,
GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE,
KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD,
MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG,
PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM,
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM,
ZW.

(25) Filing Language: Swedish

(26) Publication Language: English


(30) Priority Data:
0303064-0 19 November 2003 (19.11.2003) SE

(71) Applicant (for all designated States except US): MA-
QUET CRITICAL CARE AB [SE/SE]; Röntgenvägen
2, S-171 95 Solna (SE).

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,

[Continued on next page]

(54) Title: Method and device for reducing the carbon dioxide content in a dead volume

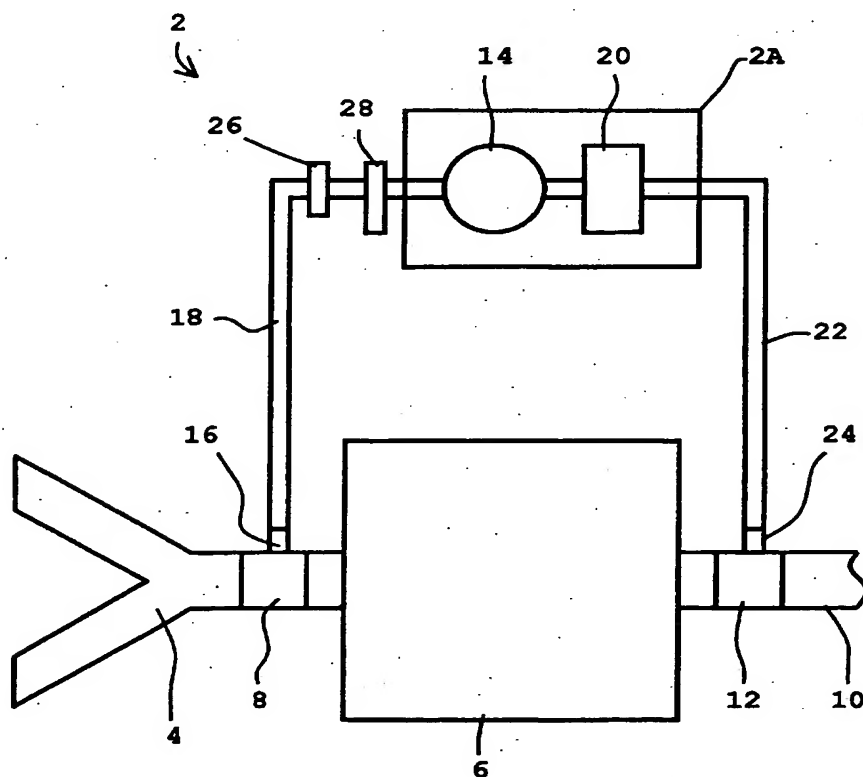

(57) Abstract: Method for reducing the carbon dioxide content in a dead volume in an apparatus designed to be connected to the respiratory system of a patient is described. The method contains the steps that, by means of a flow generator (14), a flow of gas is generated from an outlet (16) associated with the dead volume, lead the gas through a carbon dioxide absorber (20), and replace the gas which passed the absorber (20) to an inlet (24) associated with the dead volume. A device (2) is also described.



ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HU, IE, IS, IT, LU, MC, NL, PL, PT, RO, SE,
SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ,
GW, ML, MR, NE, SN, TD, TG).

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Published:

— *with international search report*